


# Model G-CEM1000 CO Monitor

## Infrared Flue Gas Analyser

The G-CEM1000 analyser uses an in-situ probe set into a duct to measure CO concentration in the flue gases. The probe includes a section that allows the diffusion of flue gases into the measurement zone or the dispersion of zero/purge air out of the tube and into the duct.

The analyser uses infrared gas cell correlation technology to determine the CO levels in the flue gases as they diffuse into the measurement chamber. The diffusion cell enables accurate measurements to be made in high flue gas dust levels exceeding several gram/m<sup>3</sup>.

- infrared flue gas analyser
- stainless steel in-situ probe
- maintenance-free operation
- high dust loading operation
- auto zero
- remote data display
- data in ppm

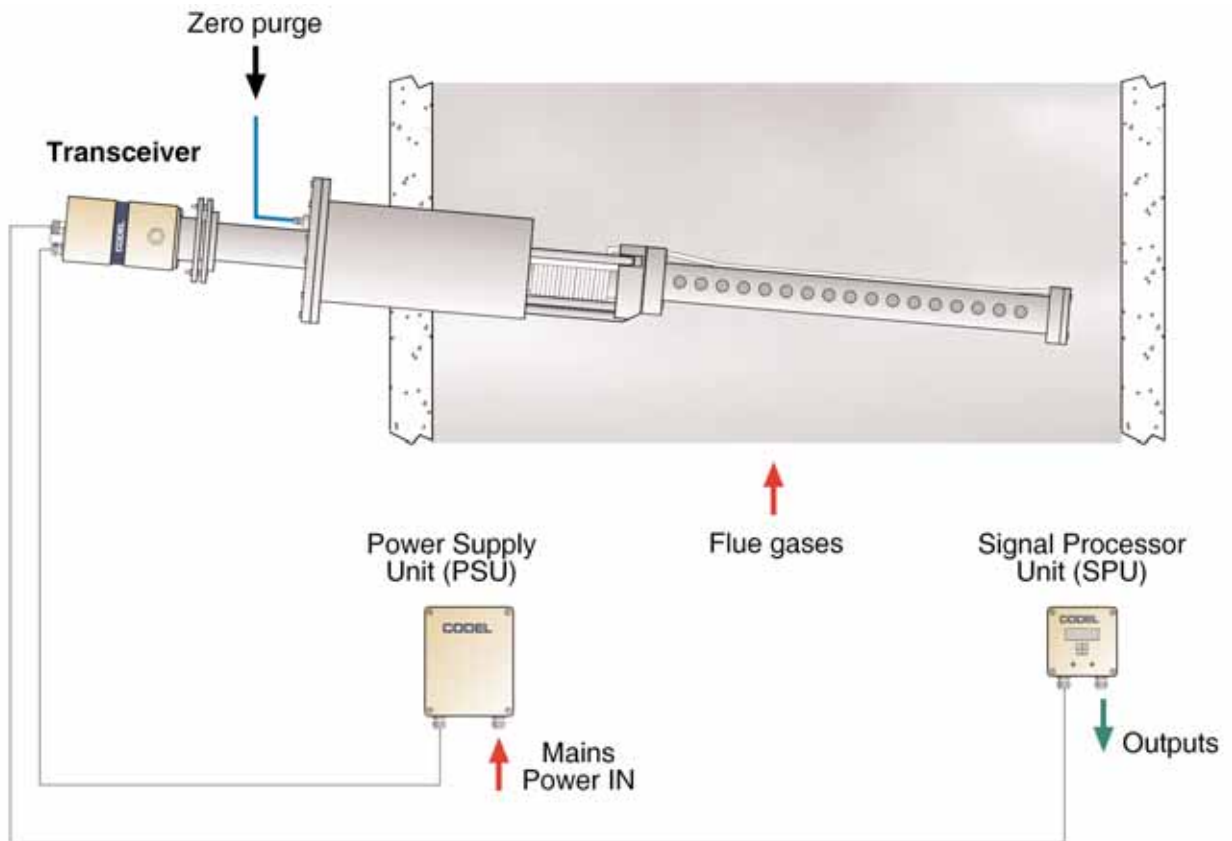


**Total Solutions - Total Confidence**

*SmartCem*



## Overall Unit Dimensions

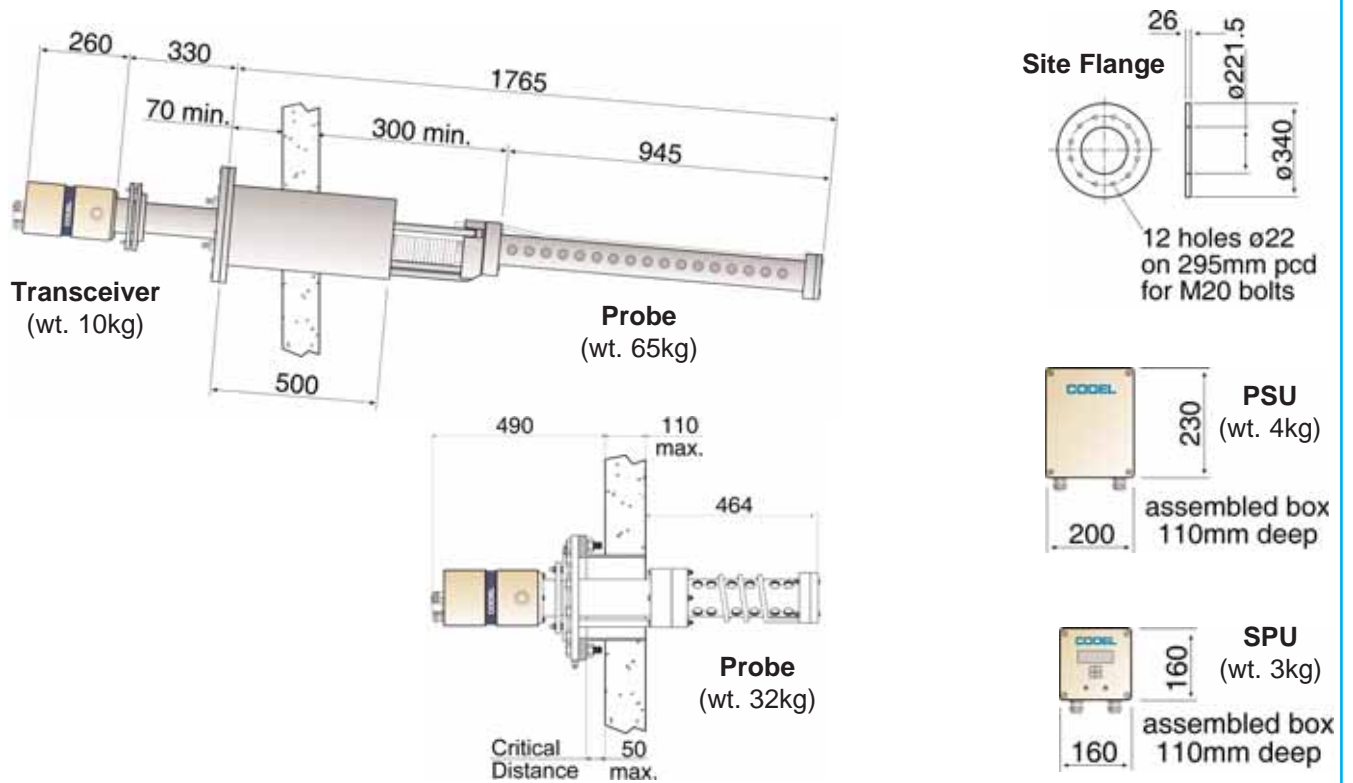

## Specification

### Measurements

Operating Principle	- infrared gas cell correlation
Span	- fully selectable in the range 0-500ppm
Averaging	- 4 rolling averages selectable from 10 seconds to 30 days
Accuracy	- $\pm 2\%$ of span
Response Time	- <200 seconds
Calibration	- auto zero

### Compliances

EMC	- 89/336/EEC directive compliant
Low Voltage	- 73/23/EEC directive compliant

### Input & Outputs

Analogue Outputs	- 2 x 4-20mA current outputs, isolated, 500 $\Omega$ load max., fully configurable from keypad
Logic Outputs	- 2 x volt-free SPCO contacts, 50V, 1A max., configurable as alarm contacts - 1 x volt-free SPCO contact, 50V, 1A max. for data valid

### General

Display	- 32-character alpha-numeric back-lit LCD
Keypad	- 4-key soft-touch entry
Construction	- epoxy-coated aluminium to IP67
Ambient Temperature	- -20°C to +50°C
Flue Gas Temperature	- 300°C max.
Power	- 76V to 265V AC @ 50/60Hz, 60VA
Calibration Air	- compressed air, 10 litre/min @ 5bar

SmartCem

CODEL International Ltd.  
Station Building, Station Road  
Bakewell, Derbyshire DE45 1GE  
England

Tel: +44 (0) 1629 814 351  
Fax: +44 (0) 8700 566 307  
e-mail: [codel@codel.co.uk](mailto:codel@codel.co.uk)  
web site: [www.codel.co.uk](http://www.codel.co.uk)

### Distributor :

